



David CHIEN et al.  
DEVICE AND METHOD FOR IN-LINE BLOOD  
TESTING USING BIOCHIPS  
Atty. Dkt. No. 072121-0371  
SN 10/733,767

BEST AVAILABLE COPY


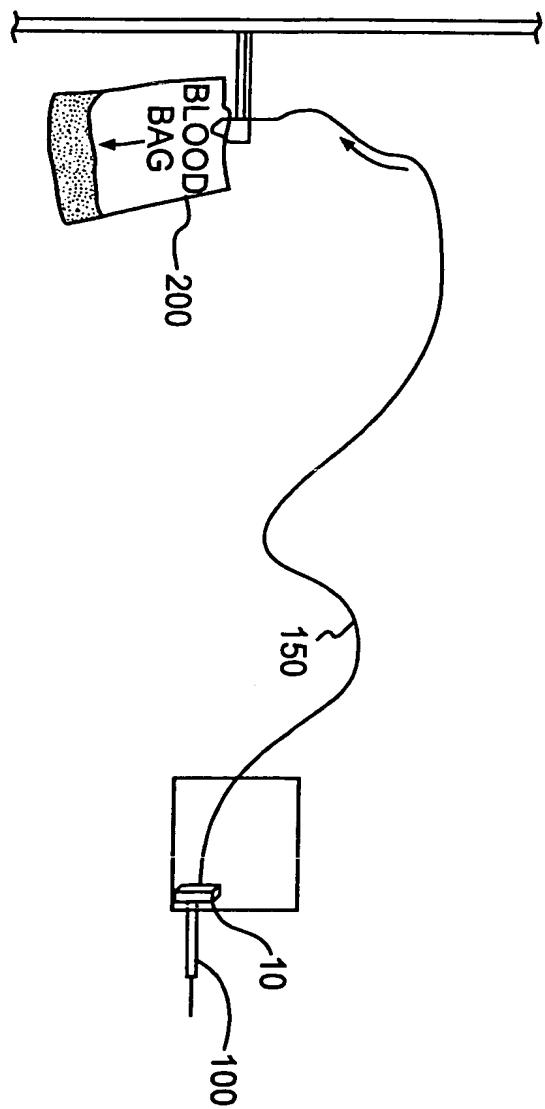


FIG. 1A

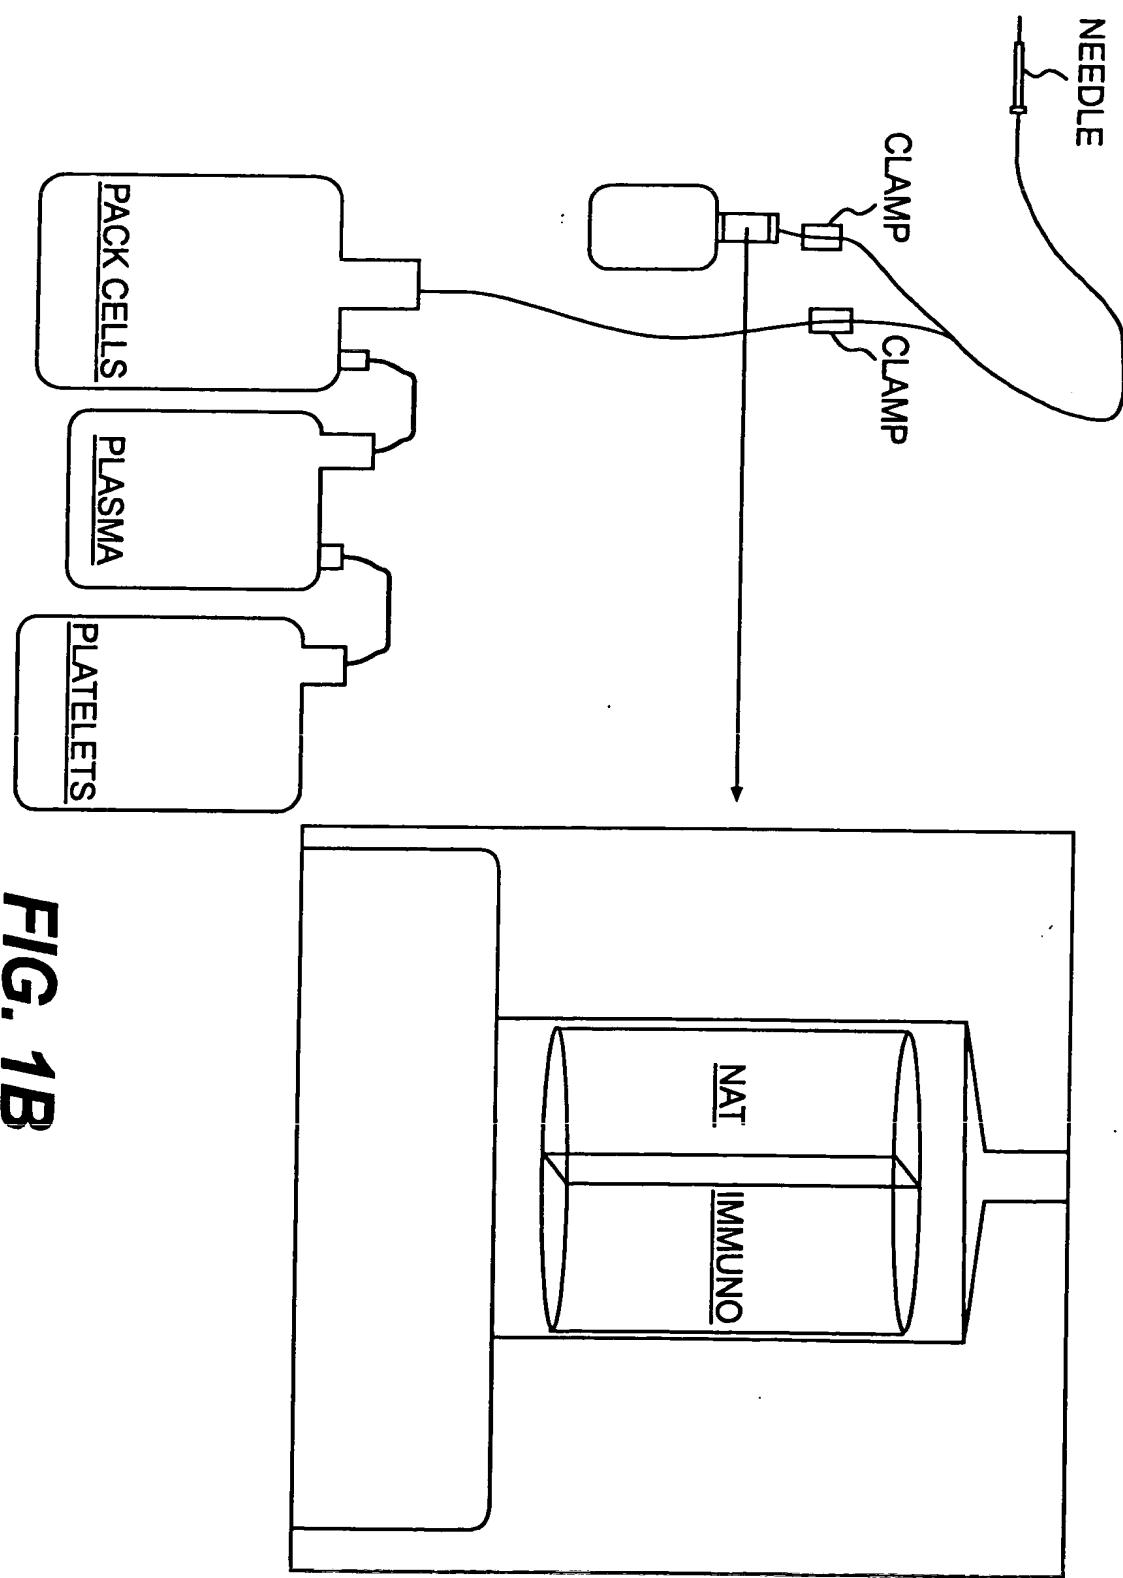

**FIG. 2**


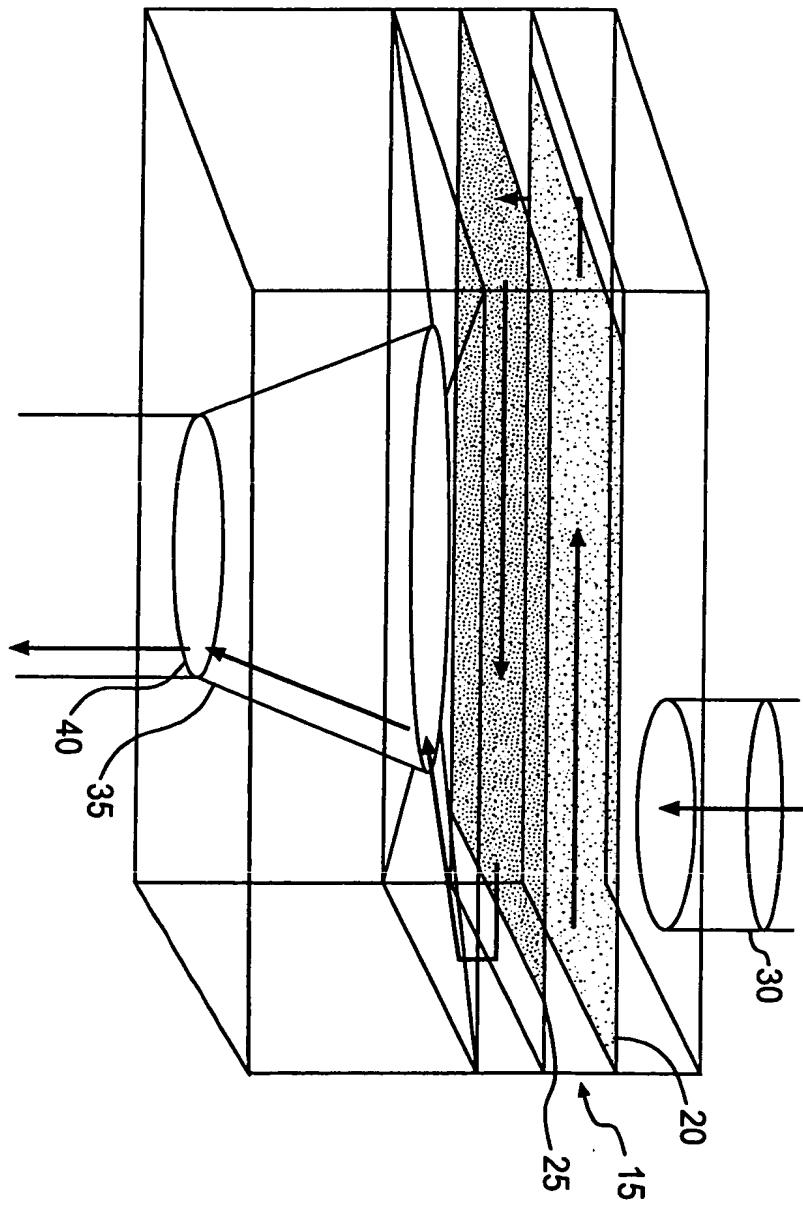


FIG.3

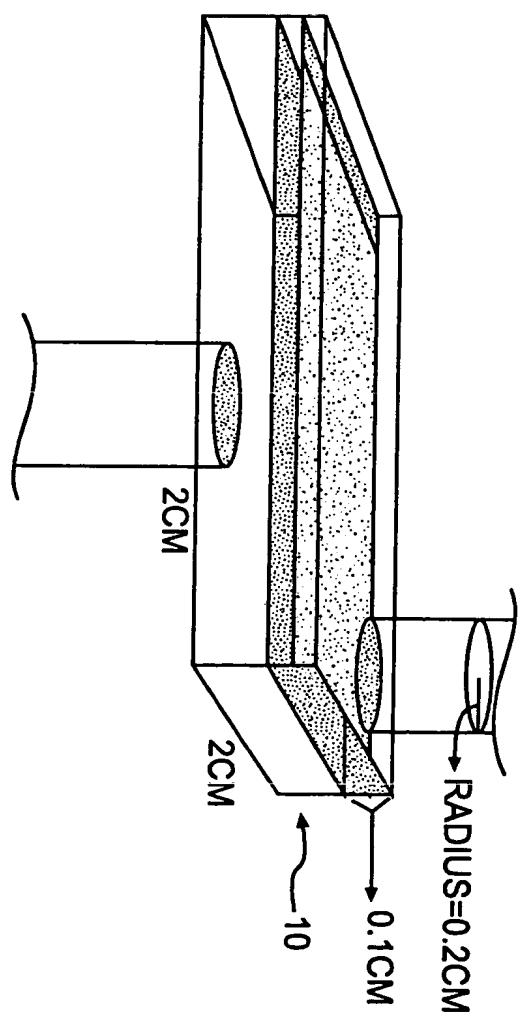

David CHIEN et al.  
DEVICE AND METHOD FOR IN-LINE BLOOD  
TESTING USING BIOCCHIPS  
Atty. Dkt. No. 072121-0371  
SN 10/733,767

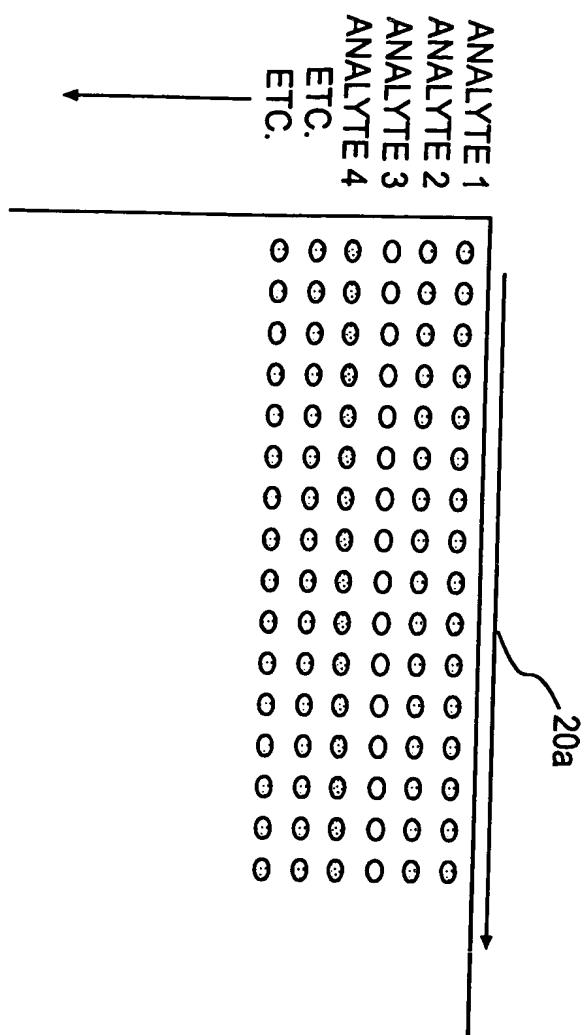
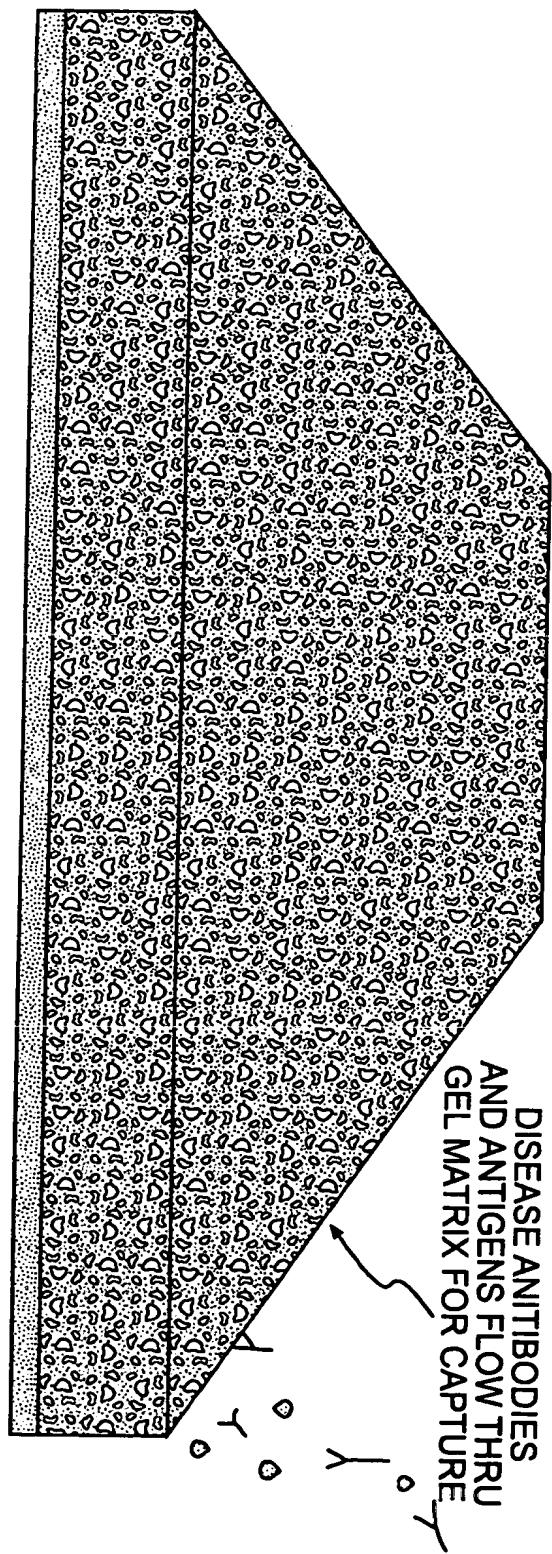


FIG. 4A

FIG. 4B




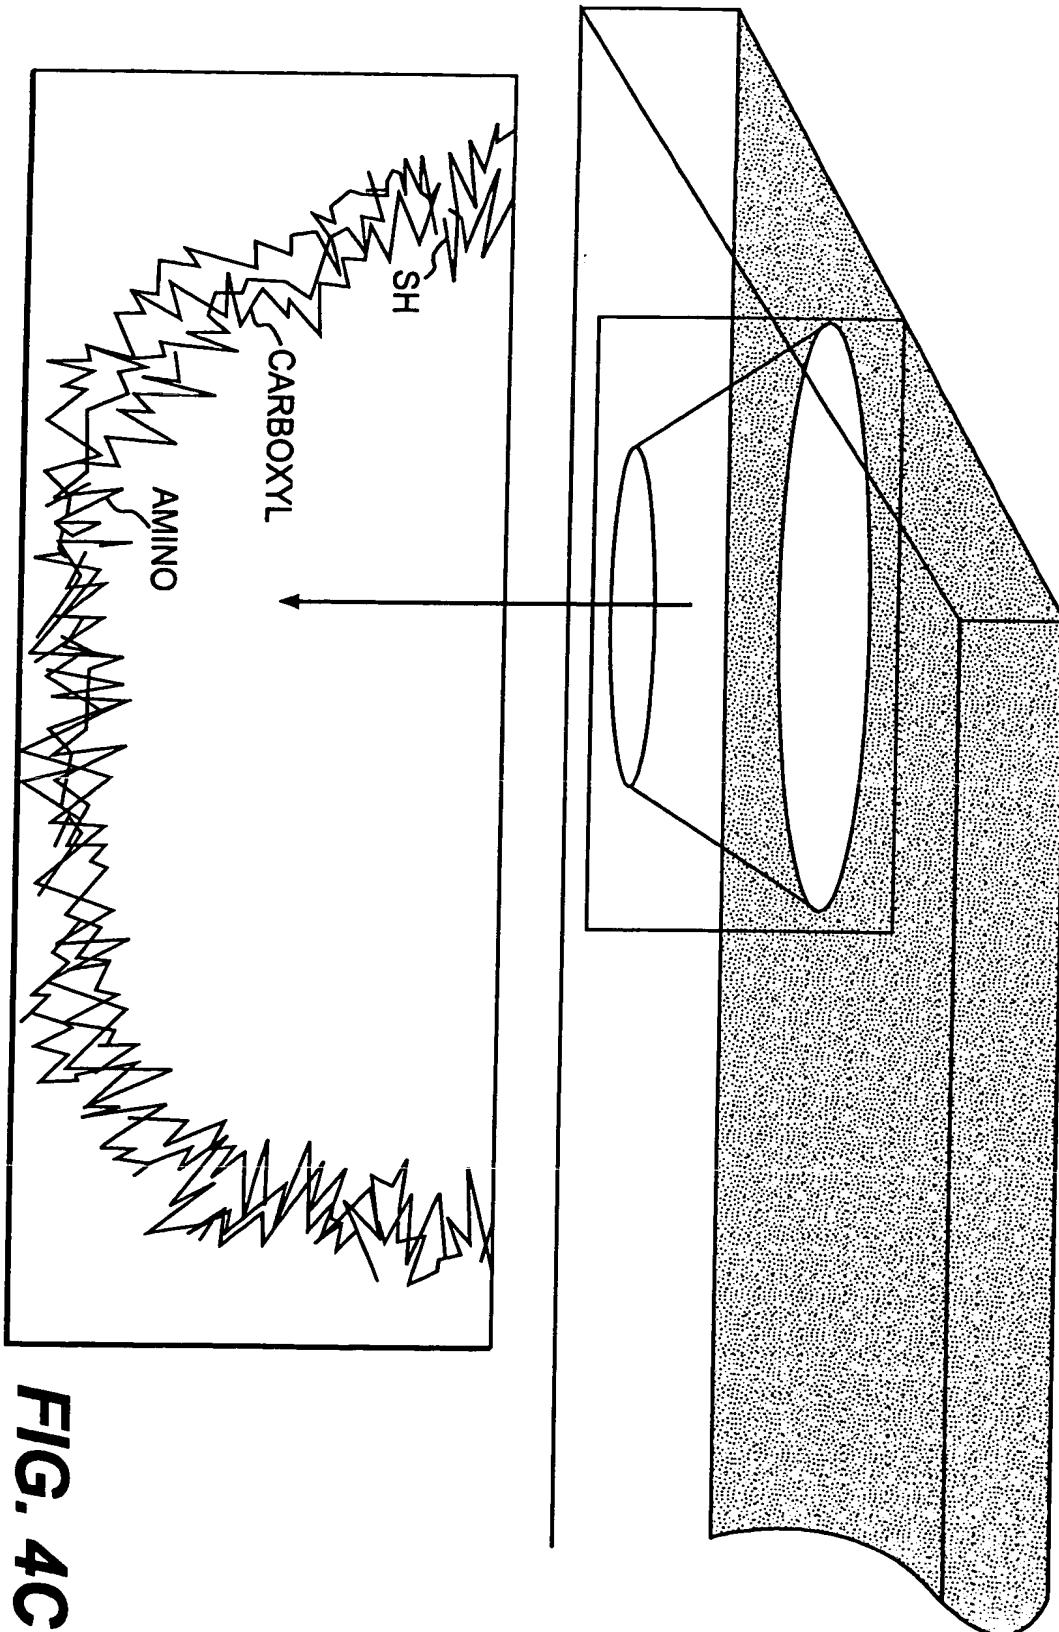



FIG. 4C


FIG. 4D

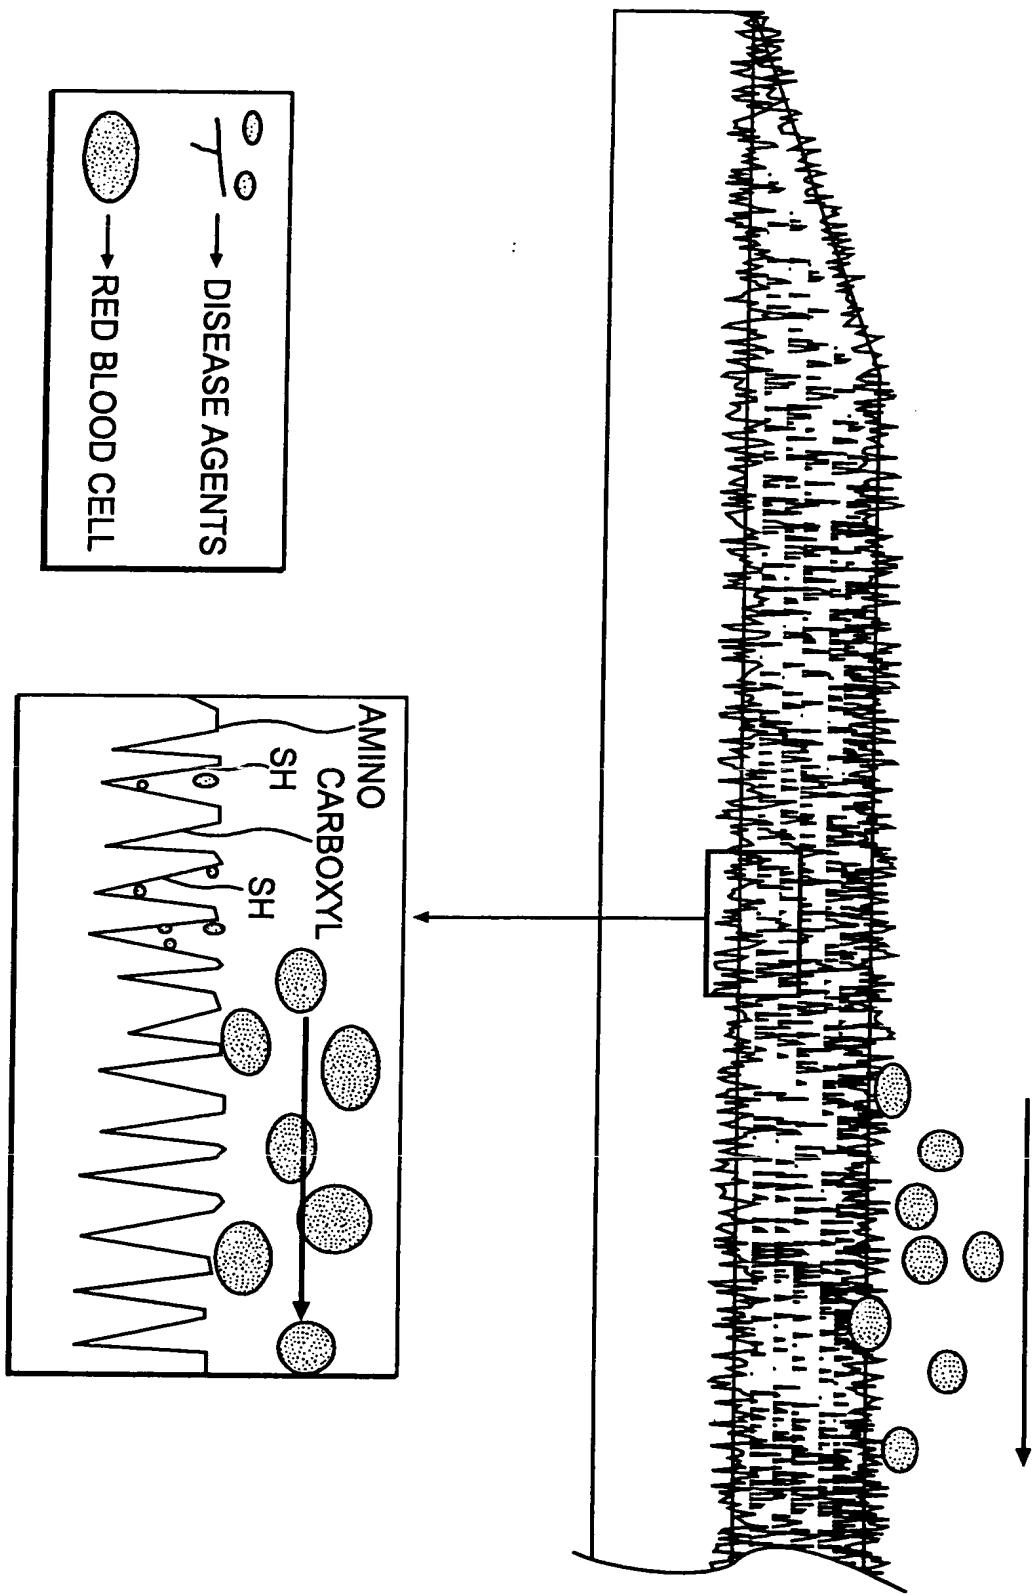


David CHIEN et al.  
DEVICE AND METHOD FOR IN-LINE BLOOD  
TESTING USING BIOCHIPS  
Atty. Dkt. No. 072121-0371  
SN 10/733,767

**FIG. 5**

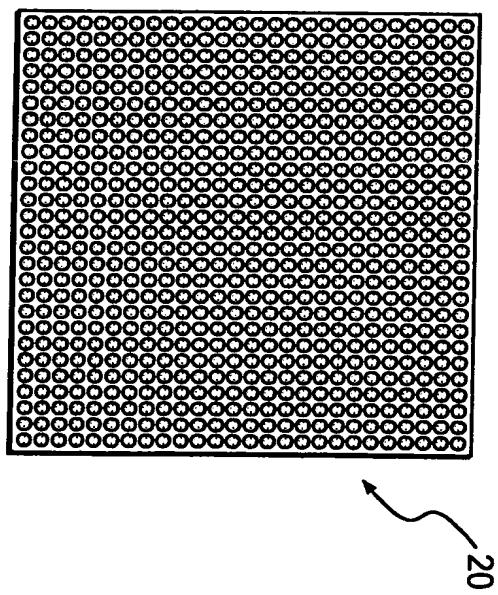


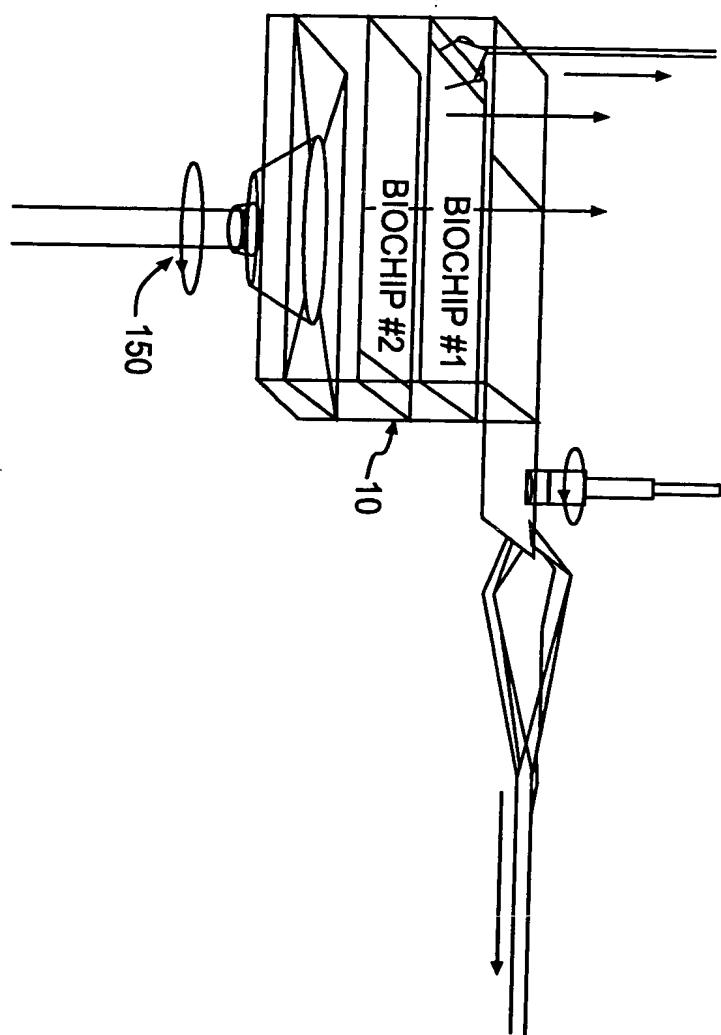

**FIG. 6**

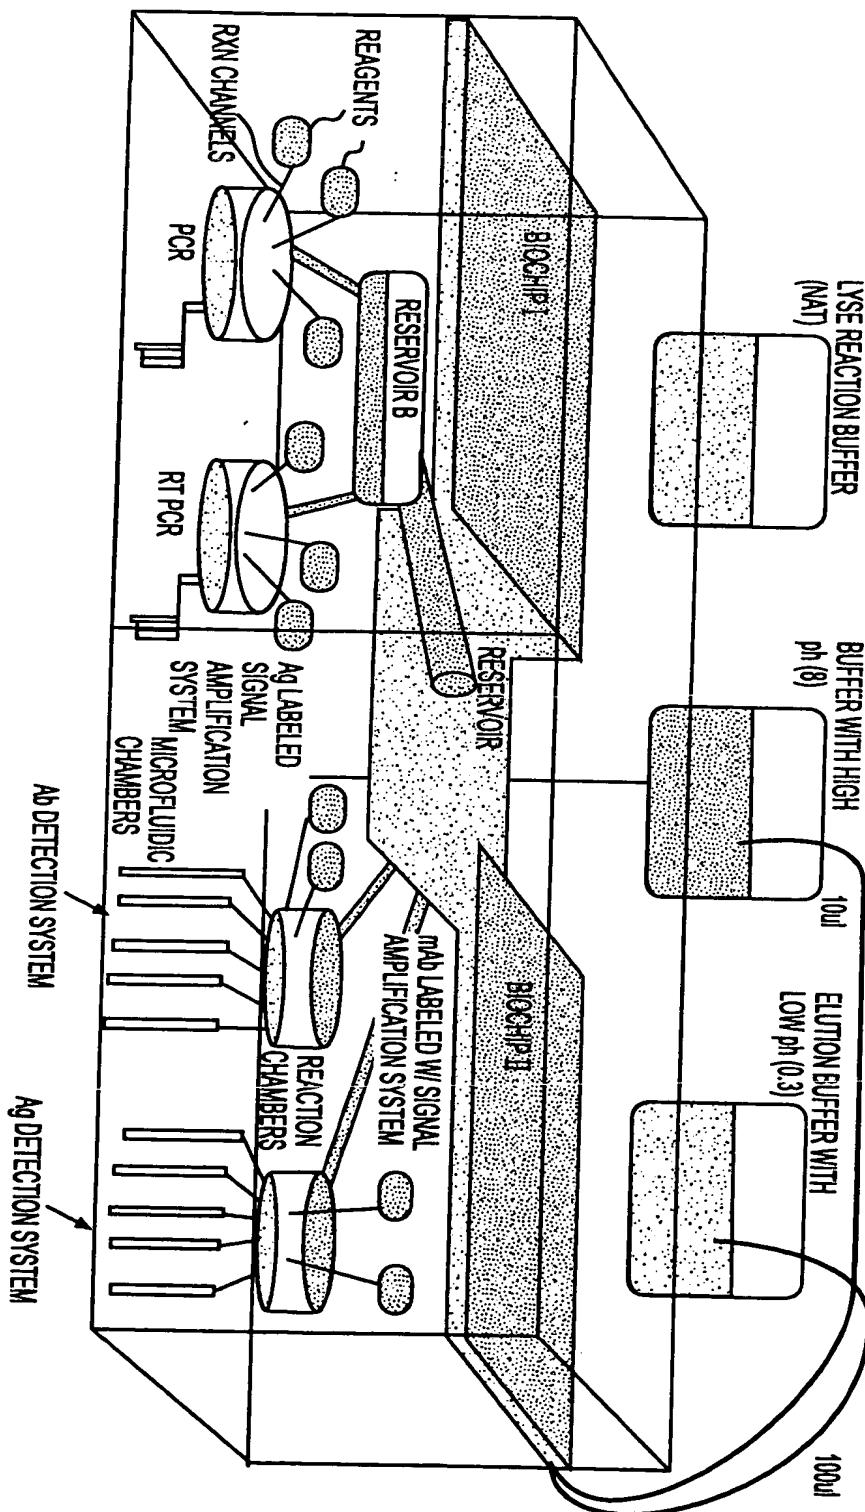



**FIG. 7A**

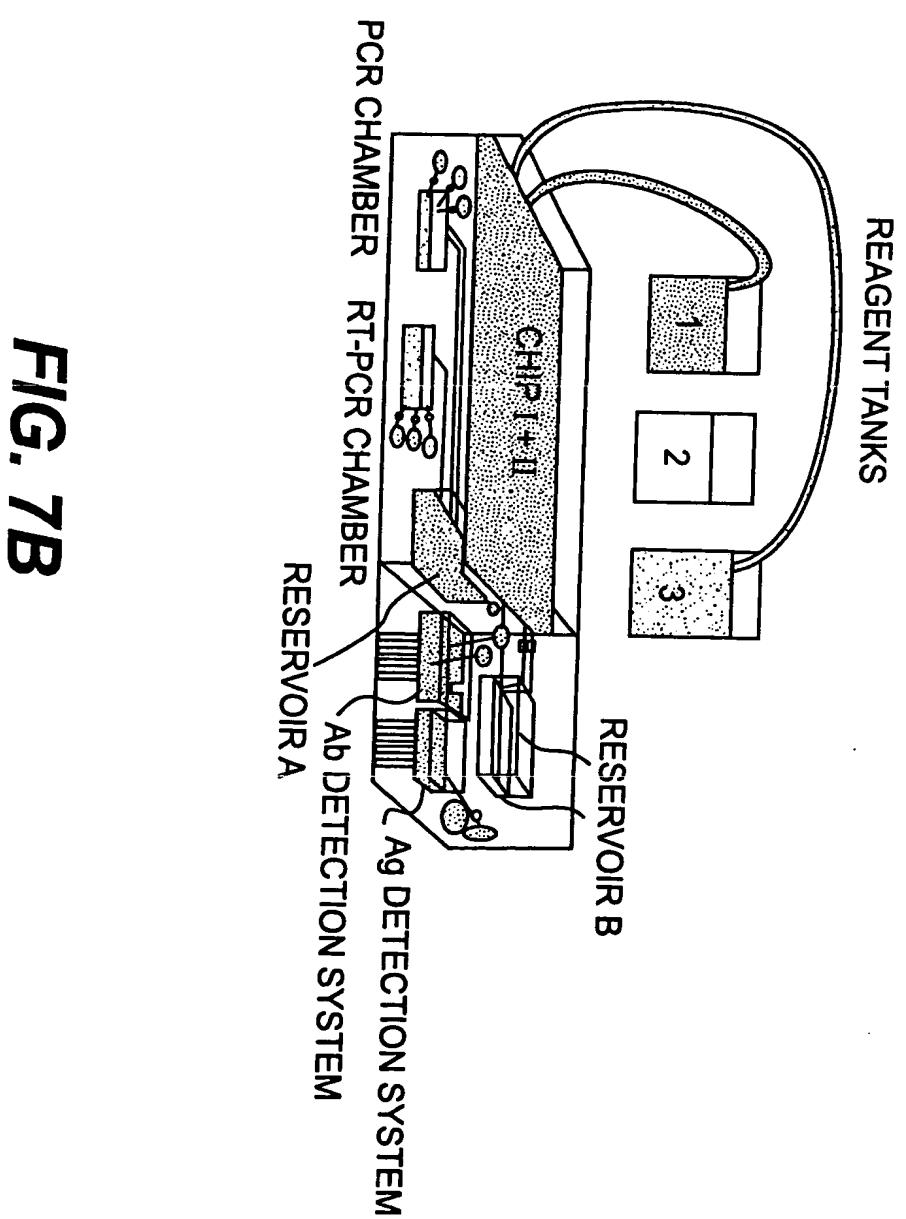


**FIG. 7B**

*FIG. 8*

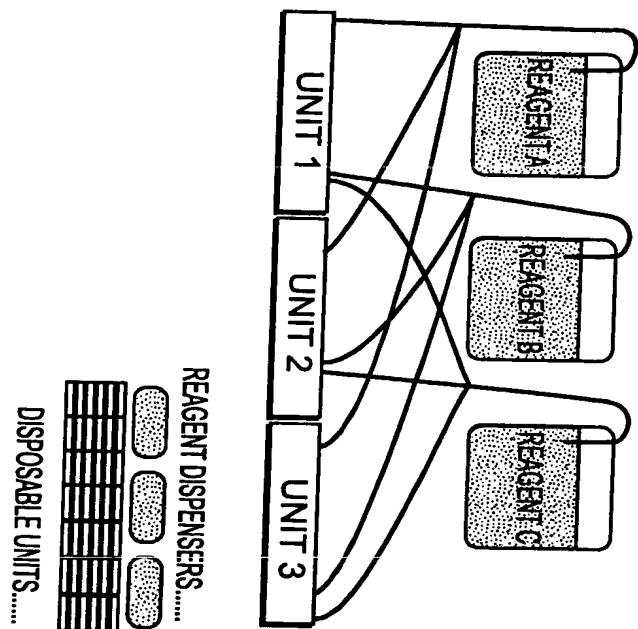


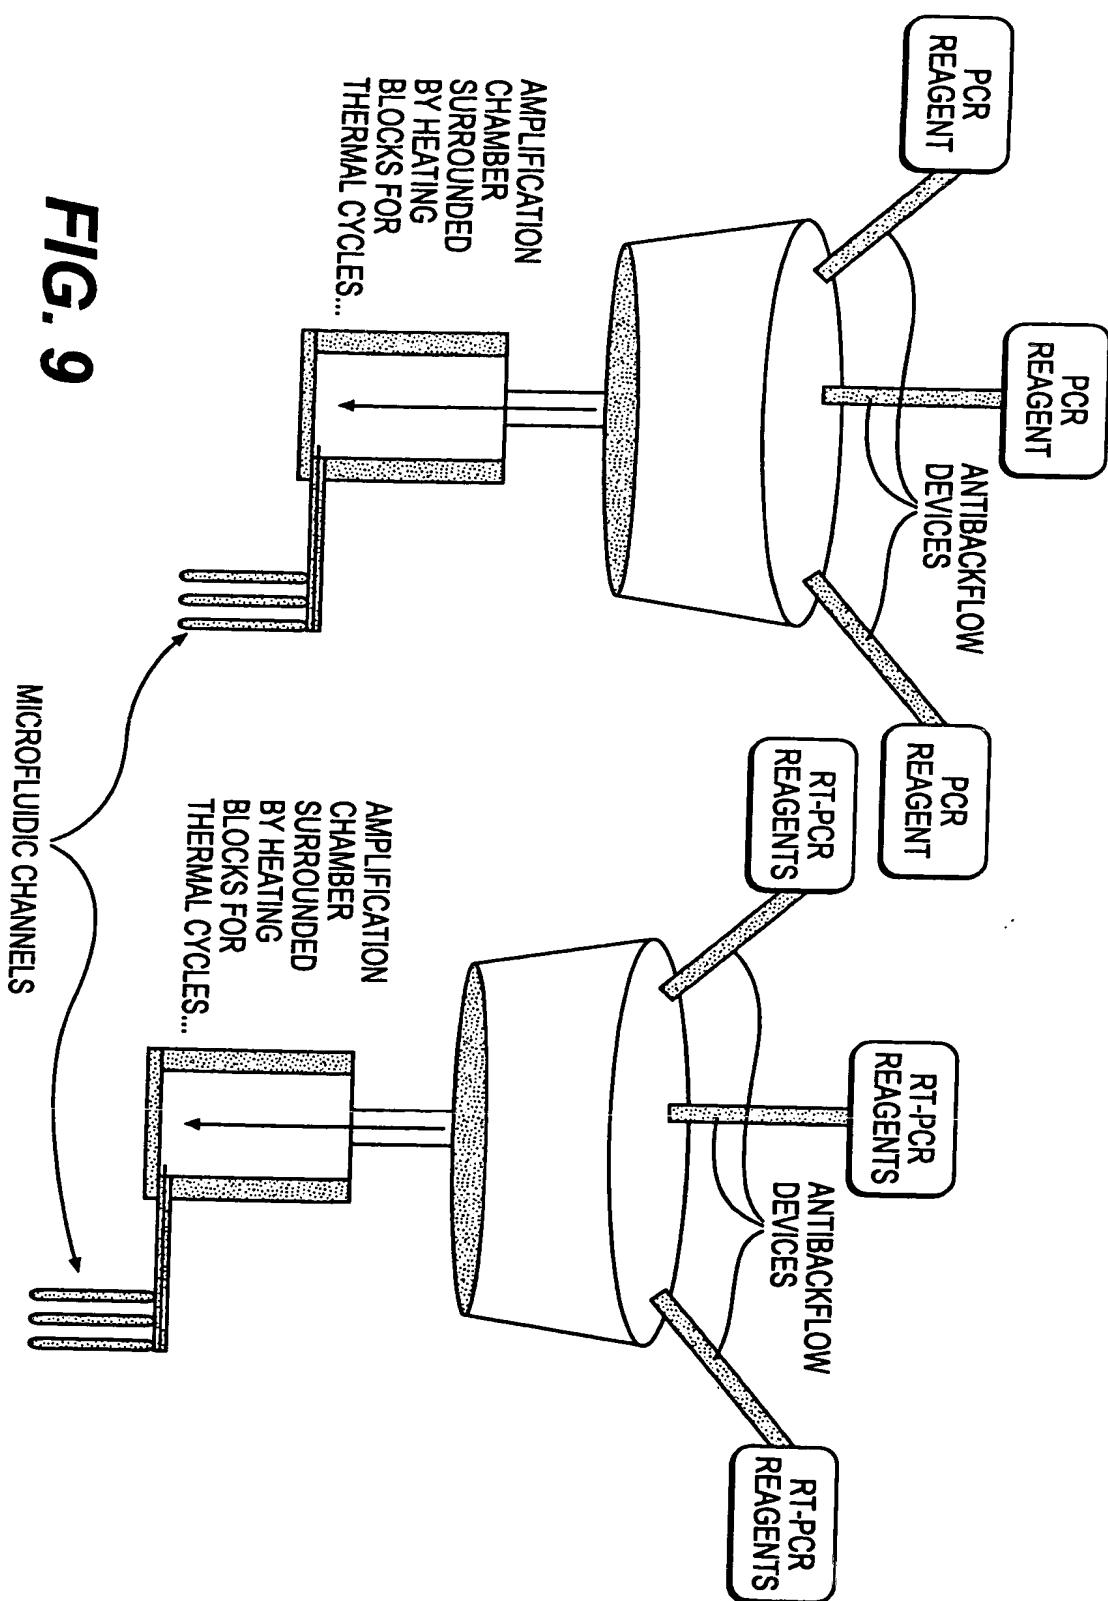

David CHIEN et al.  
DEVICE AND METHOD FOR IN-LINE BLOOD  
TESTING USING BIOCCHIPS  
Atty. Dkt. No. 072121-0371  
SN 10/733,767

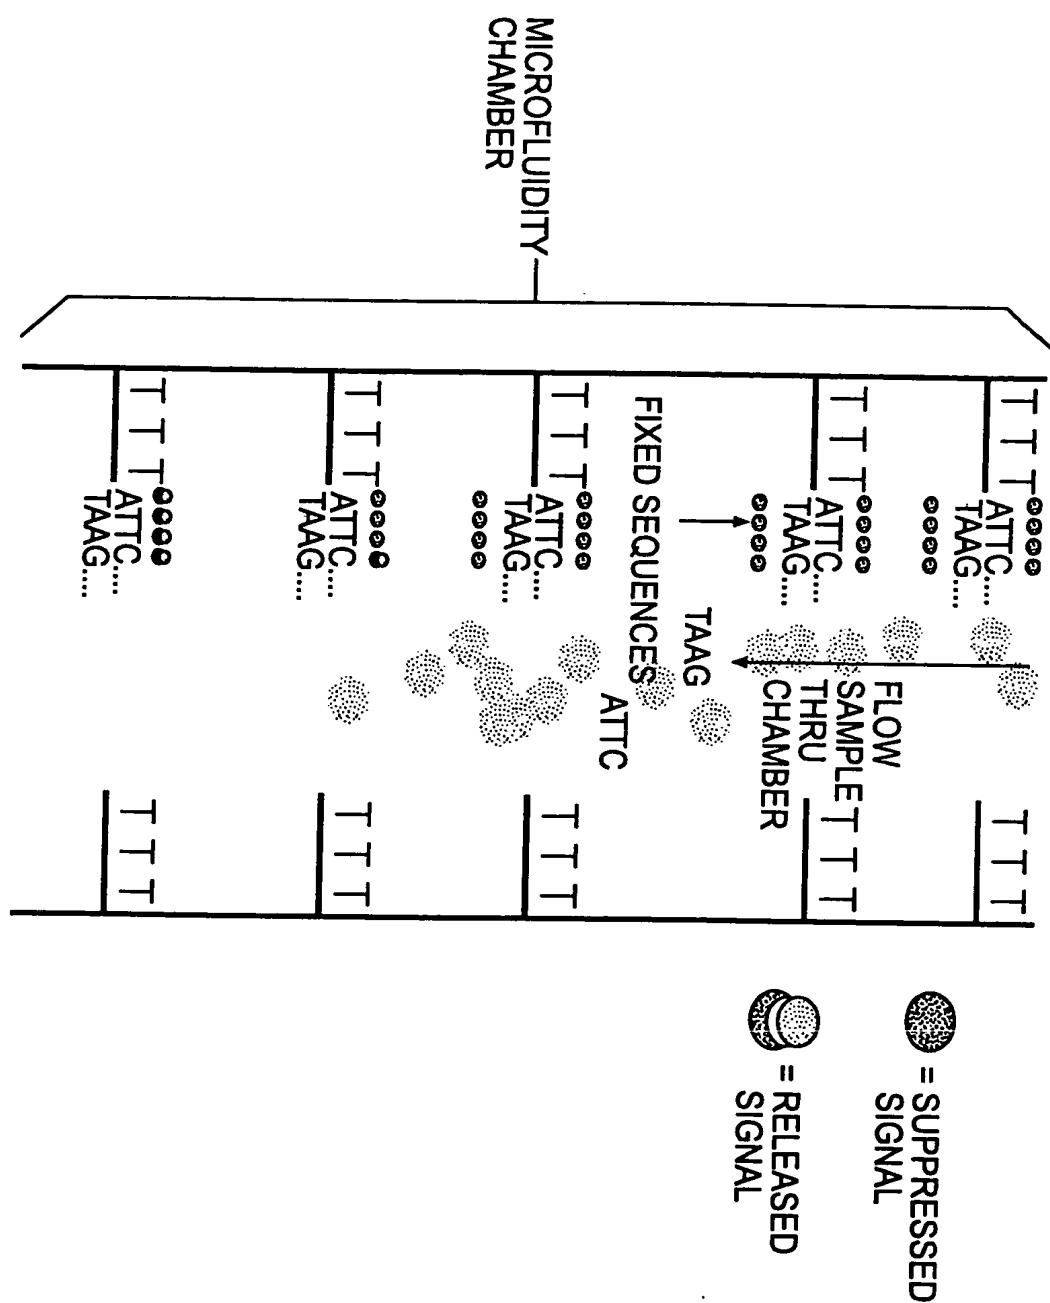



**FIG. 10**

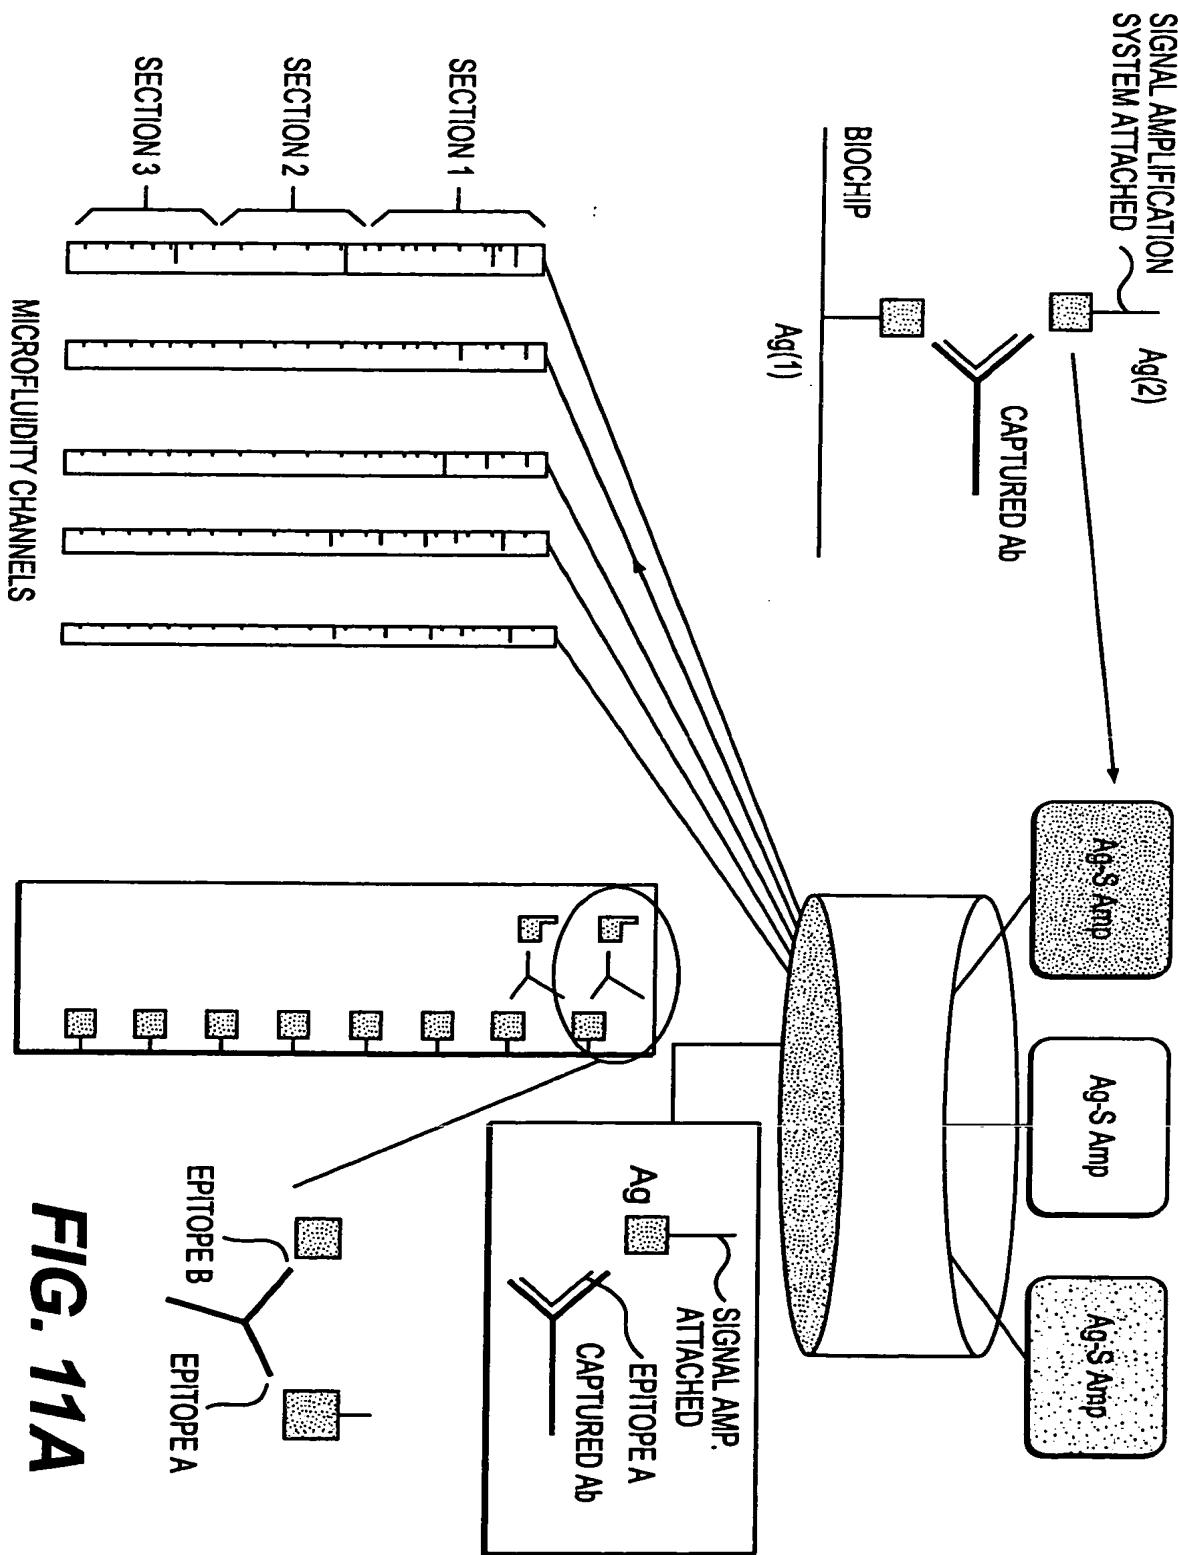


**FIG. 11A**

**FIG. 11B**

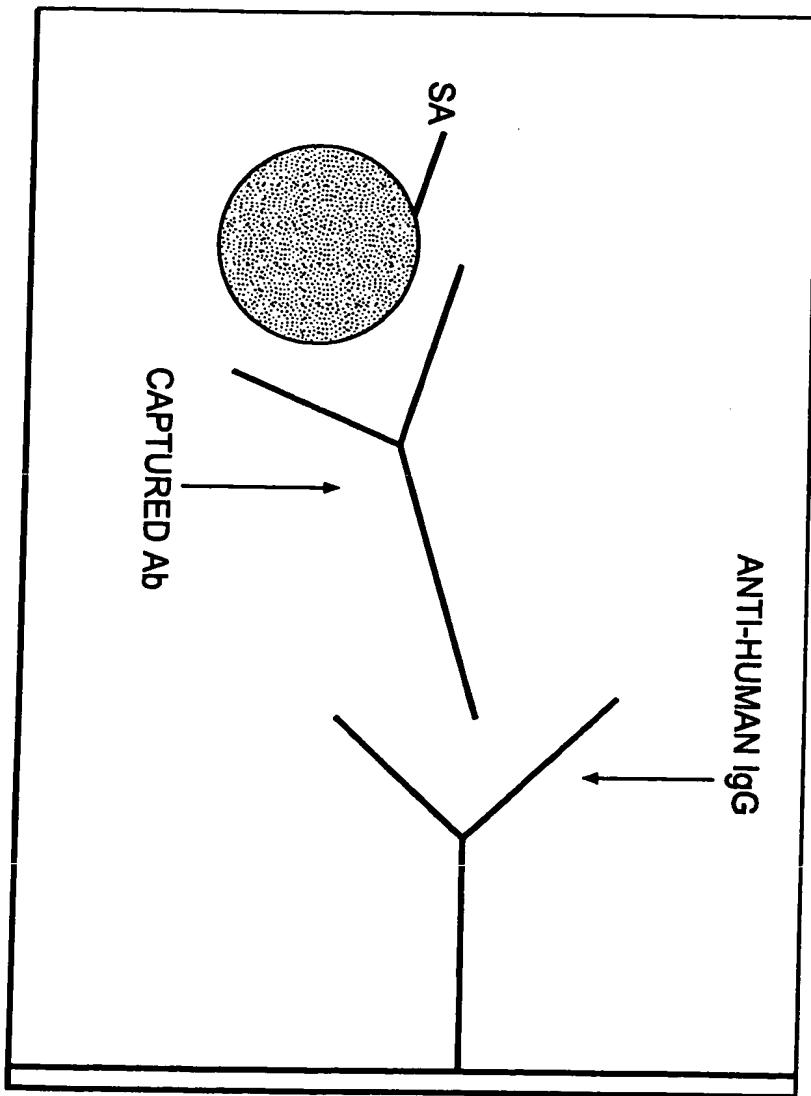

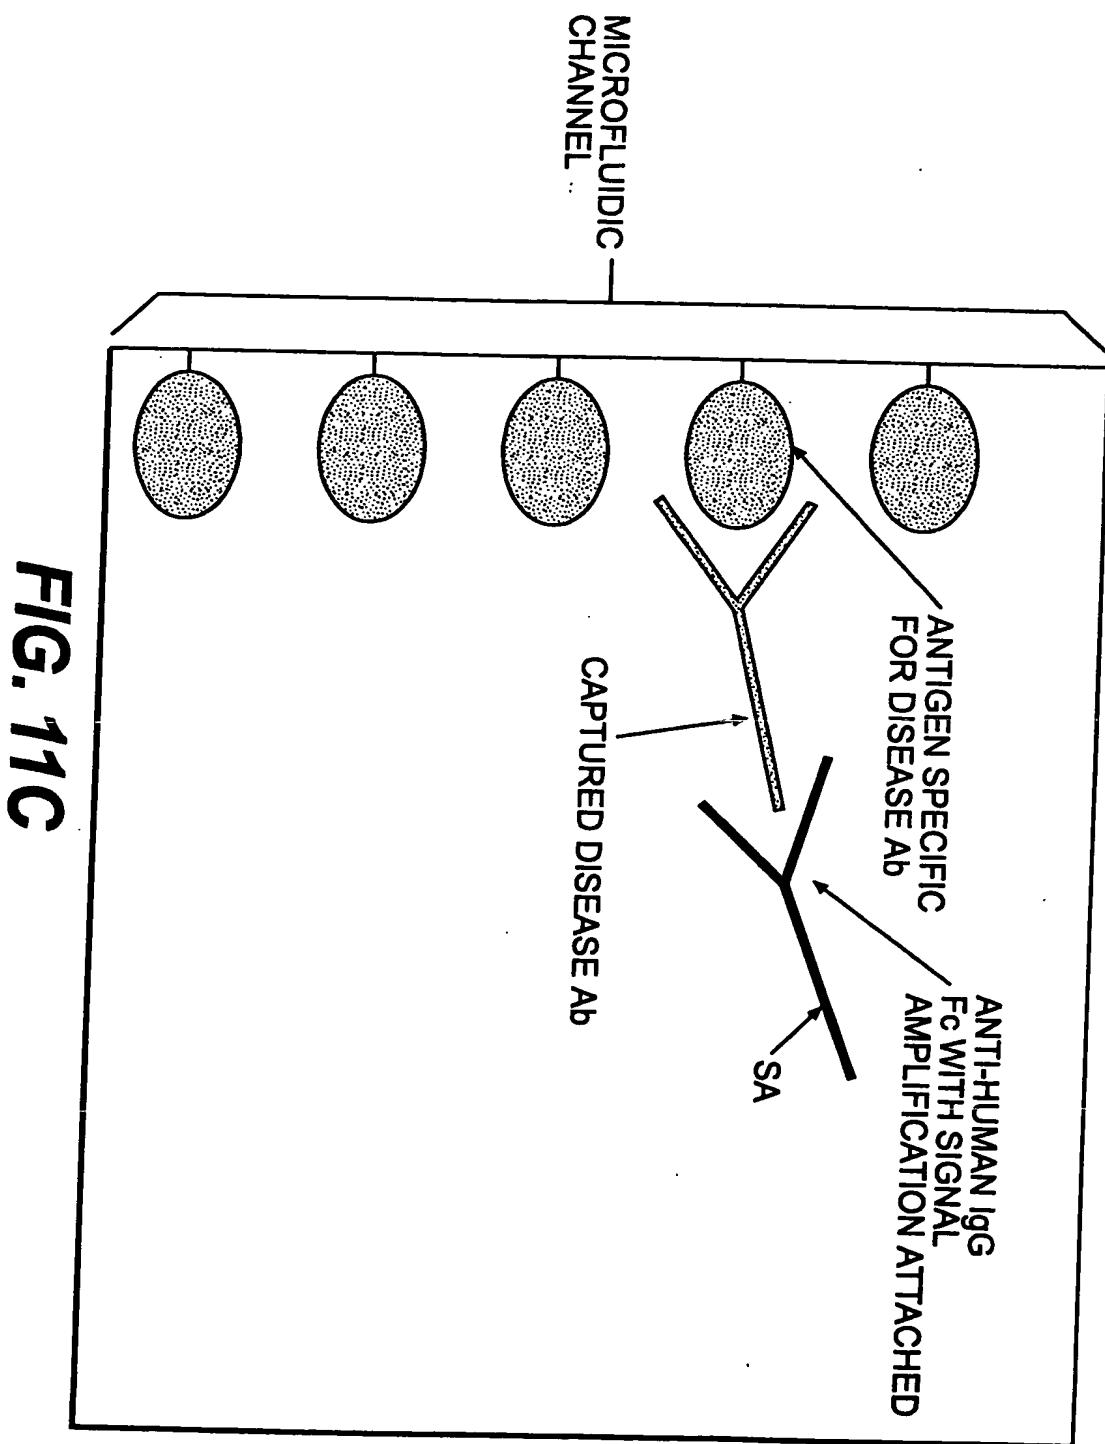

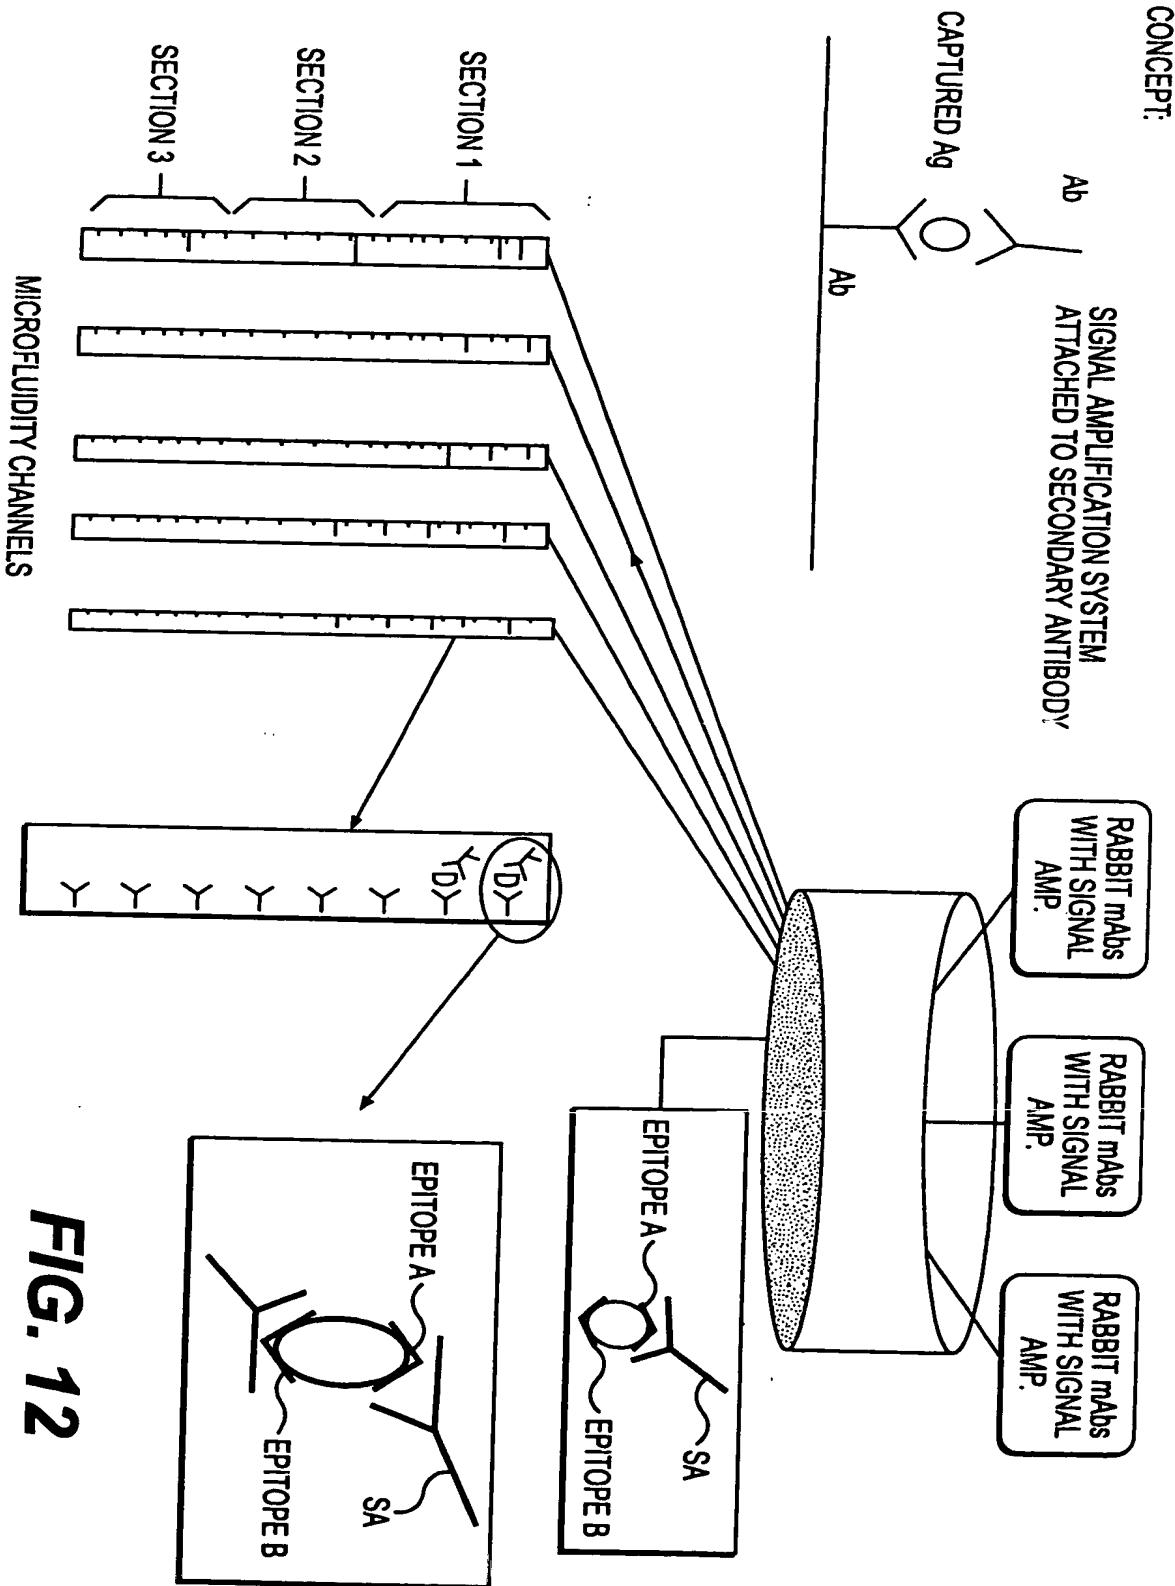



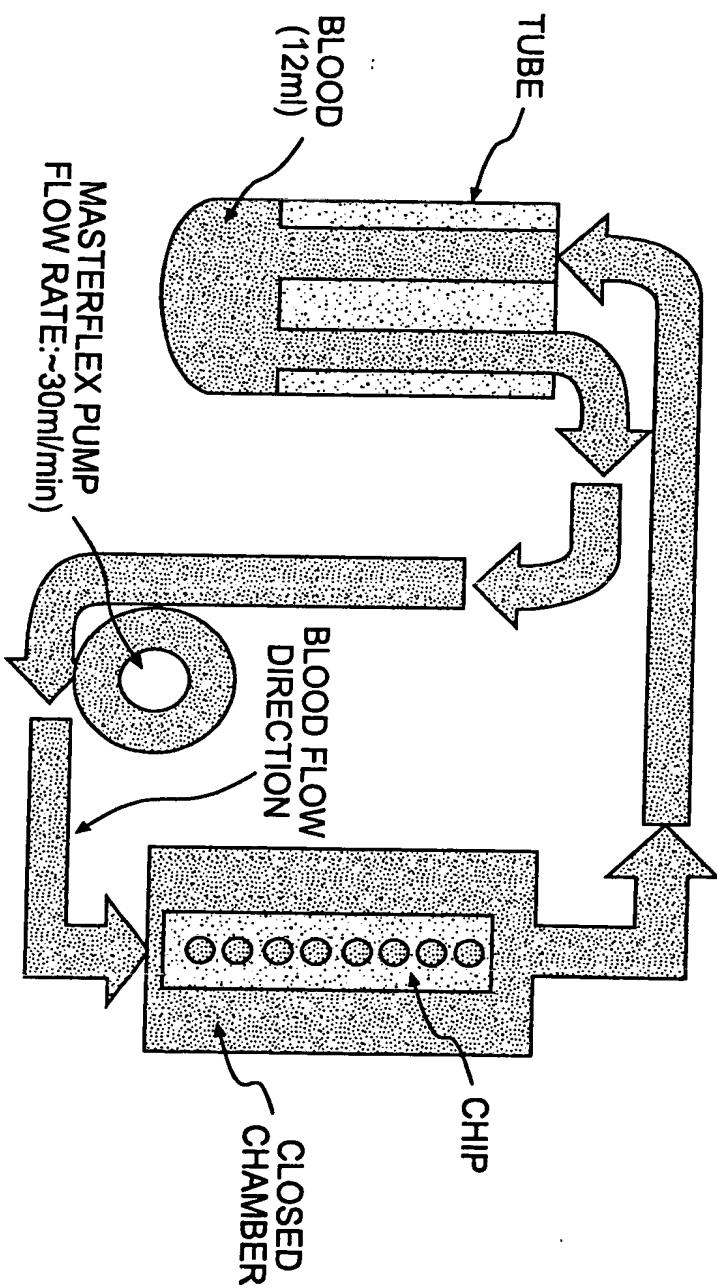


FIG. 13

David CHIEN et al.  
DEVICE AND METHOD FOR IN-LINE BLOOD  
TESTING USING BIOCIPS  
Atty. Dkt. No. 072121-0371  
SN 10/733,767

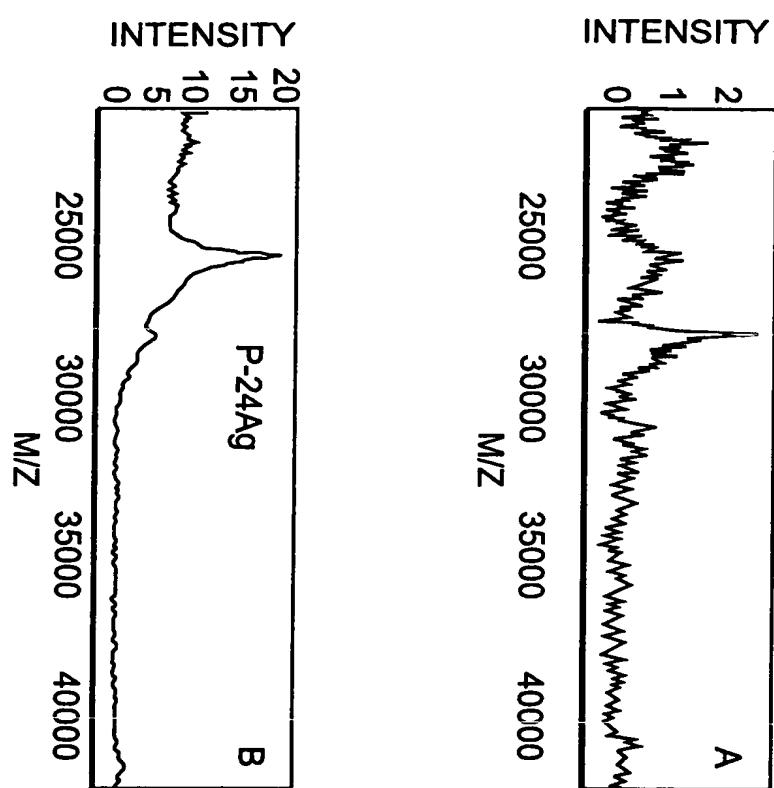

*FIG. 14*

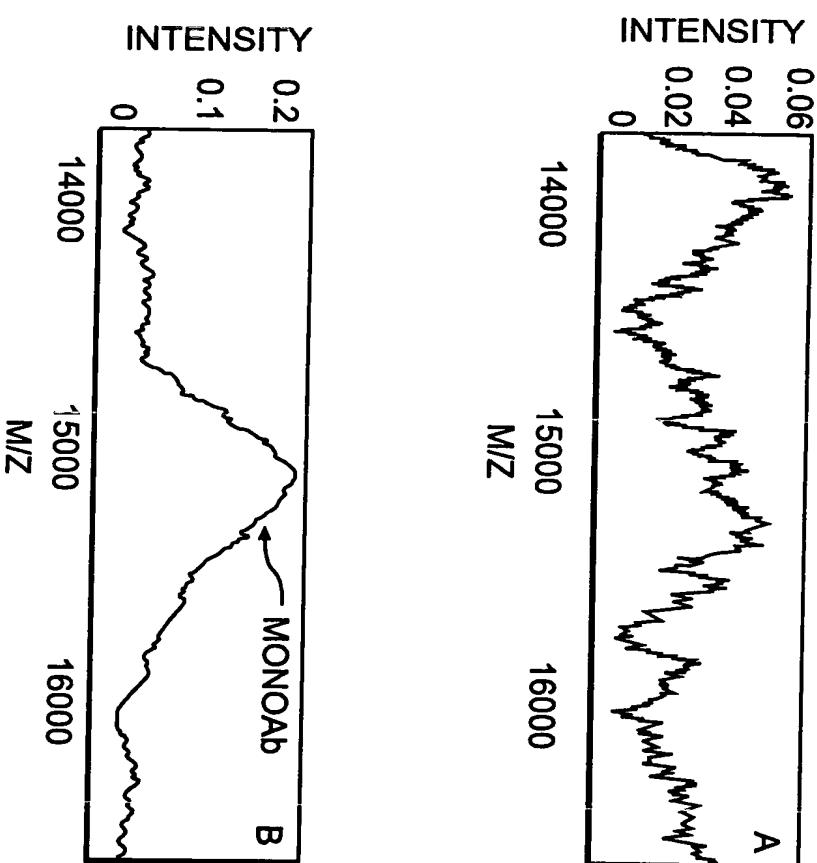

**FIG. 15**

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

## **BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- BLACK BORDERS**
- IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- FADED TEXT OR DRAWING**
- BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- SKEWED/SLANTED IMAGES**
- COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- GRAY SCALE DOCUMENTS**
- LINES OR MARKS ON ORIGINAL DOCUMENT**
- REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- OTHER:** \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**